




Calibration spectrum from ^{137}Cs :

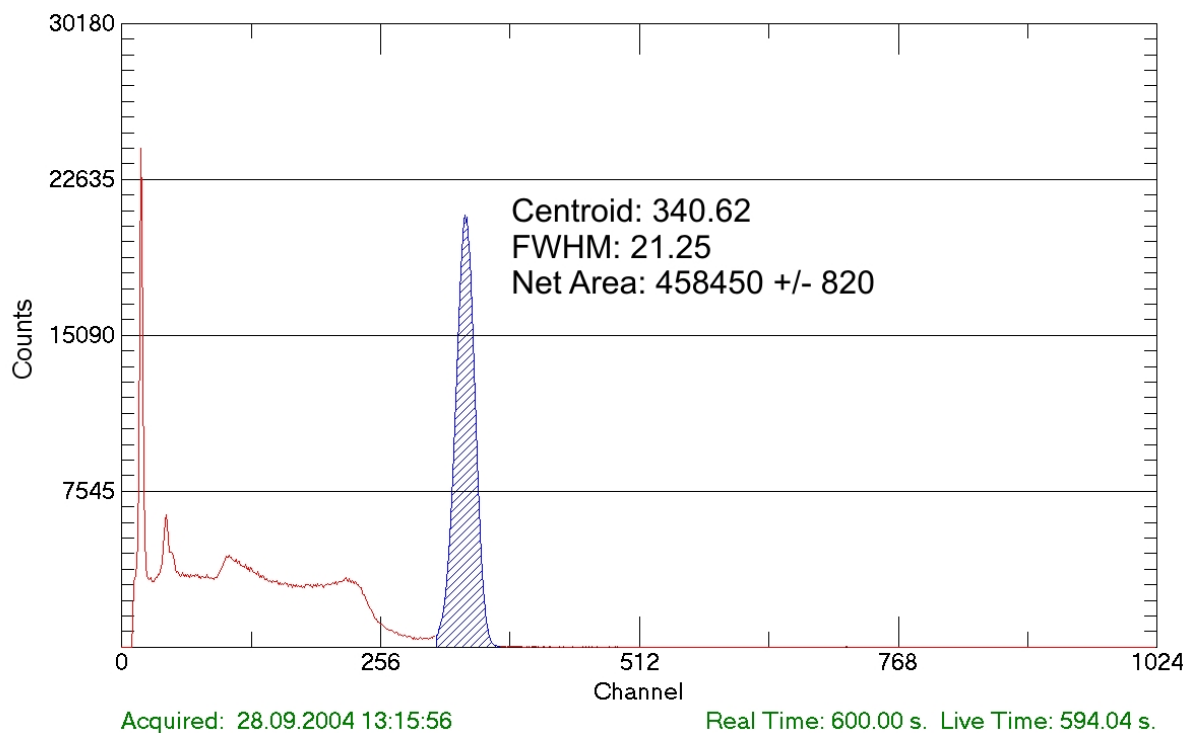


Calibration spectrum from ^{88}Y :

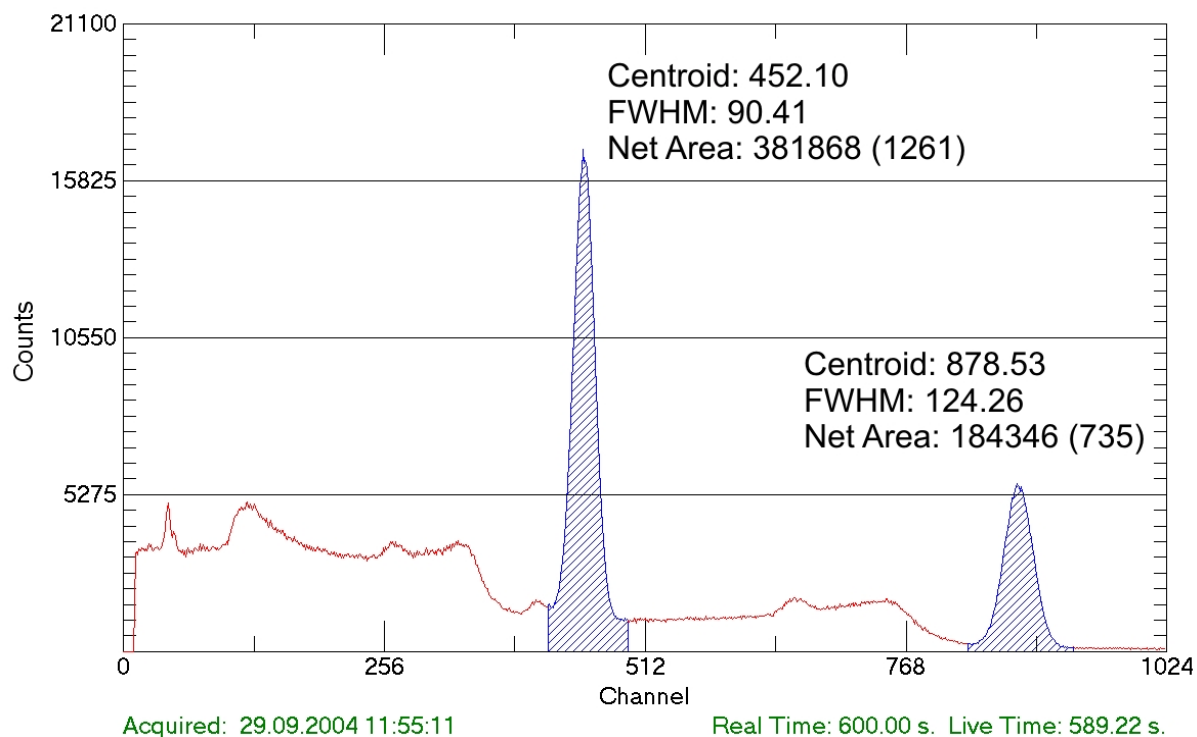


Calibration spectrum from ^{60}Co :

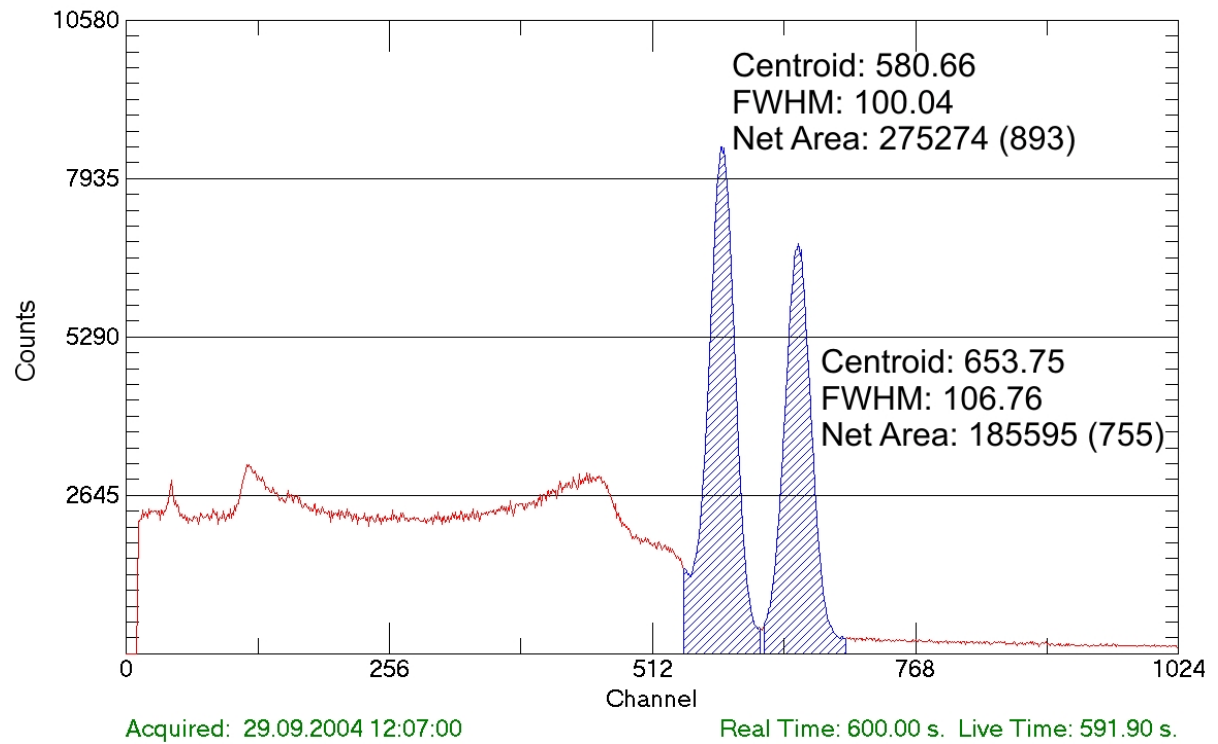


Calibration spectrum from ^{241}Am :

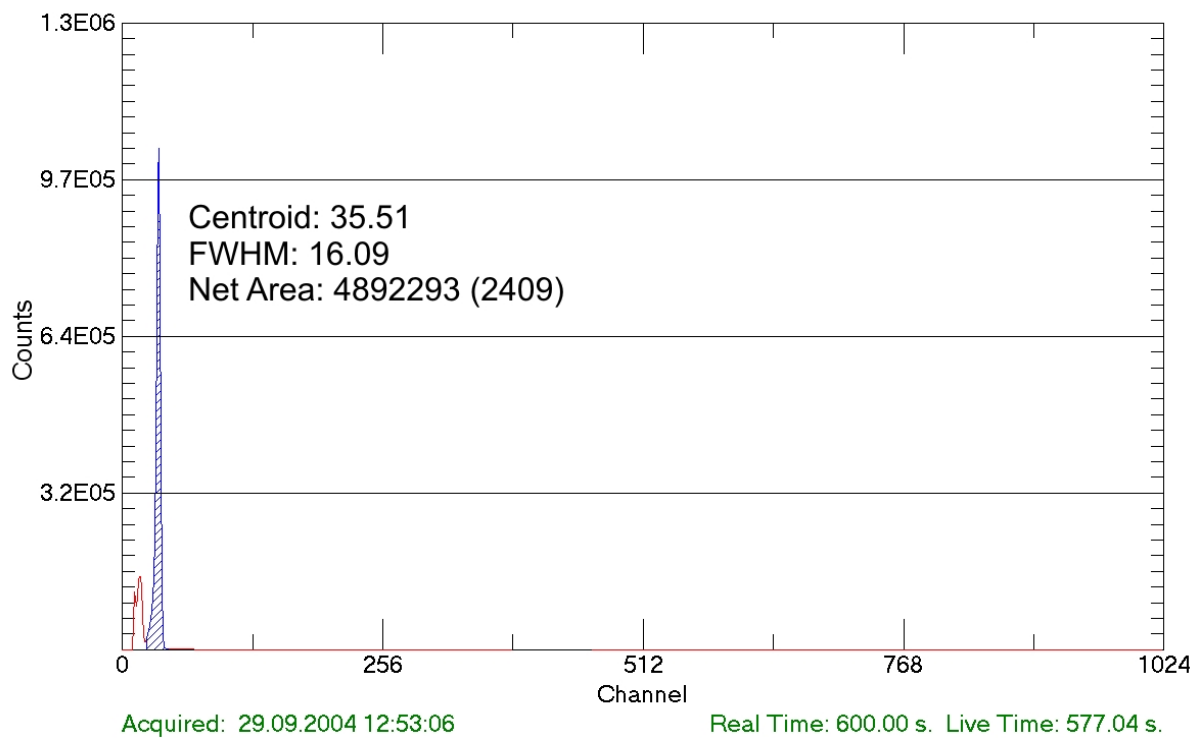


Calibration spectrum from ^{54}Mn :

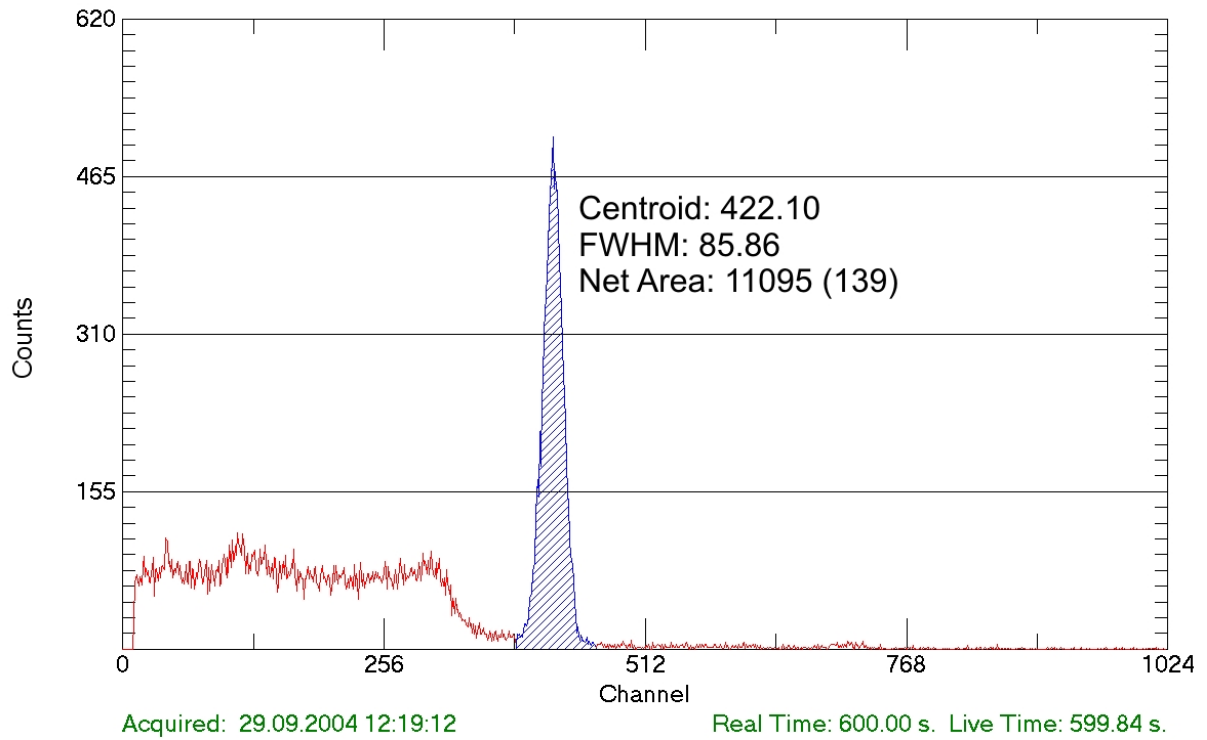

Calibration spectrum from ^{133}Ba :

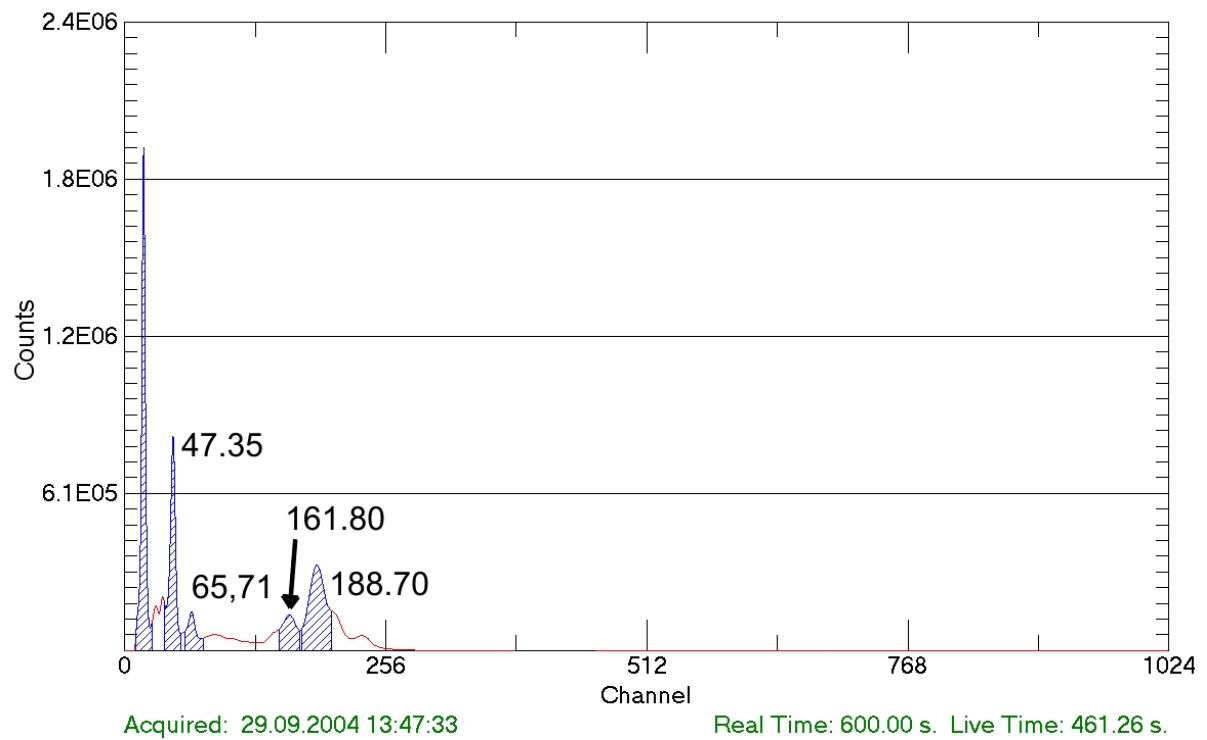

Spectrum from unknown sample 1:

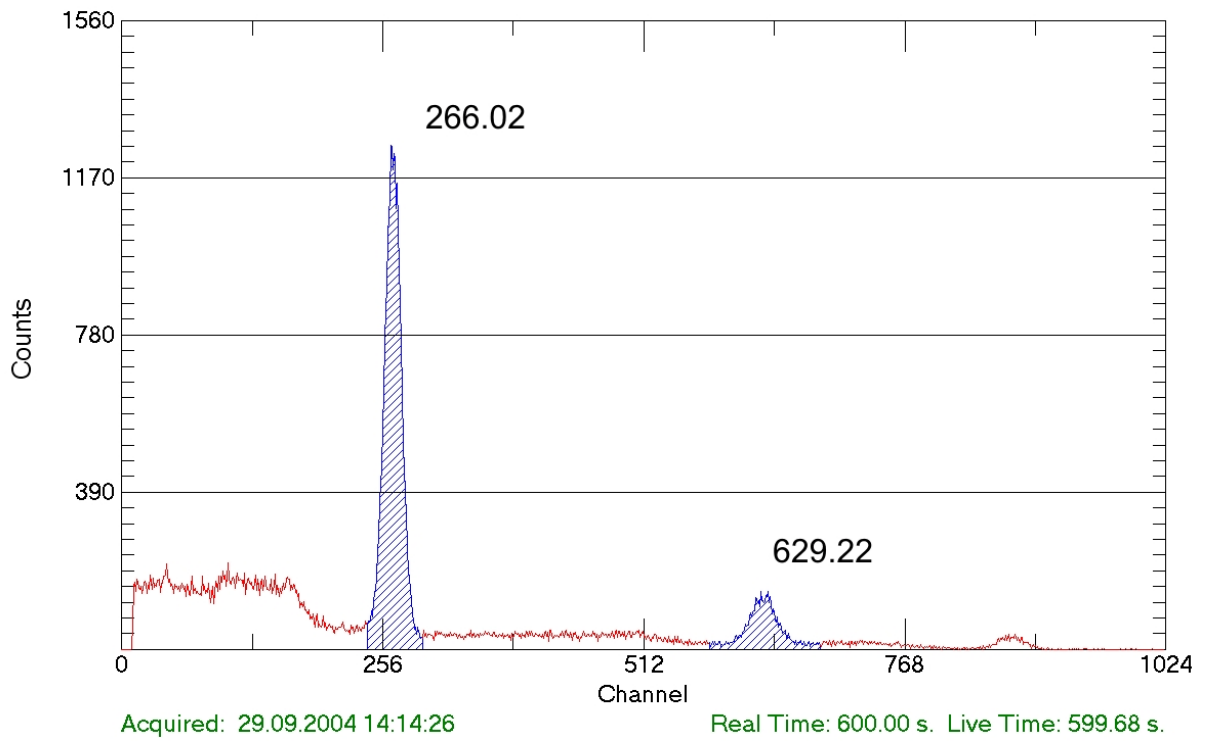

Spectrum from unknown sample 2:

